

|  |  |
|--|--|
| <b>Product PN</b> GSS021A00S                                     | <b>Mod. 984e-ext</b><br><b>Rev. 07</b> |
| <b>Description</b> HI-FLO Extension Set Endotoxins Adult 0.2+ µm |  |

## HI-FLO Extension Set Adult with 0.2 µm Filter positively charged



|                                   |  |
|-----------------------------------|--|
| <b>PRODUCT DESCRIPTION</b>        | <p>Infusion extension set for infusion for intravascular applications.</p> <p>The device is sterile and can be used in combination with an infusion set or an infusion device (pump or syringe). The connections are a female luer lock with cap inlet and a male luer lock with 1.2 µm filter outlet, compliant with ISO 80369-7</p> <p>The set is provided with a vented Speedflow® Adult filter, with an hydrophilic PES membrane with 0.2 µm pore size positively charged for particles retention and a hydrophobic PTFE membrane with 0,03 µm pore size.</p> <p>The approximate total length of the set is 245 mm.</p> <p>The set includes the following components:</p> <ul style="list-style-type: none"> <li>▪ Female luer lock with cap inlet;</li> <li>▪ Speedflow Adult 0.2+ µm IV Filter;</li> <li>▪ Male luer lock with filter outlet.</li> </ul>                                   |
| <b>MANUFACTURER NAME</b>          | <p><b>GVS SpA</b><br/>Via Roma, 50<br/>40069 Zola Predosa (BO) – ITALY<br/>Phone: +39.051.6176311 – Fax: +39.051.6176200<br/>e-mail: <a href="mailto:gvs@gvs.it">gvs@gvs.it</a> – website: <a href="http://www.gvs.com">www.gvs.com</a></p>  |
| <b>INTENDED USE / APPLICATION</b> | <p>Infusion of Drugs (including chemotherapy), Anesthetics, Nutritional Solutions and Saline Solutions for intravascular applications.</p> <p>The set can be connected via Luer Locks to all commercially available infusion administration sets compliant with ISO 80369-7.</p> <p>The set can be used either for gravity or in combination with an infusion set or an infusion device (pump or syringe).</p> <p>The set is intended specifically to eliminate air bubbles and to retain particles, bacteria and endotoxins.</p> <p>The set is a single-use device that can be used applications that last up to 120 hours.</p> <p>The set has to be disposed after each therapy.</p> <p>The set cannot be used for infusion of hyper alimentation liquids, lipids, blood and/or blood derivatives.</p> <p>The device should only be supervised and used by qualified healthcare personnel.</p> |
| <b>CLASS OF THE PRODUCT</b>       | <p>Class IIa – sterile – single use<br/>Rule 2 and 3 Annex VIII 2017/472/UE</p>  |
| <b>EMDN</b>                       | <p>A03020101      LOW PRESSURE EXTENSION LINES</p>   |
| <b>MATERIALS</b>                  | <p><b>Filter media:</b> PES Hydrophilic membrane / PTFE Hydrophobic membrane / Polyethylenimine<br/><b>Filter housing:</b> MBS<br/><b>Tubes:</b> PU<br/><b>Luer Lock:</b> MABS<br/><b>Caps:</b> HDPE</p> <p><b>Regulatory Compliance:</b></p> <ul style="list-style-type: none"> <li>▪ Biocompatibility according to ISO 10993-1</li> <li>▪ Rohs directive 2011/65/UE</li> <li>▪ DEHP plasticizer Free</li> <li>▪ Latex free</li> <li>▪ Reach 1907/2006/CE (hazardous substances regulation)</li> <li>▪ Reg. 1272/2008/CE (classification, labelling and packaging of substances and mixtures)</li> </ul>  |



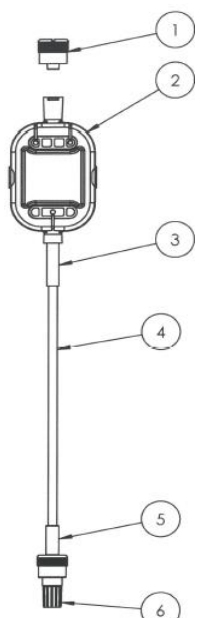
# PRODUCT SPECIFICATION



|  |  |
|--|--|
| <b>Product PN</b> GSS021A00S                                     | <b>Mod. 984e-ext</b><br><br><b>Rev. 07</b> |
| <b>Description</b> HI-FLO Extension Set Endotoxins Adult 0.2+ µm |  |

|   |   |
|---|---|
| <b>PRODUCT CHARACTERISTICS</b>              | <b>Physical/Mechanical:</b><br><b>Approximate total length:</b> 245 mm<br><b>Total internal volume of the set:</b> 5 ml<br><b>Weight:</b> 16 g<br><b>Input/output connectors:</b> Female luer lock with cap inlet compliant with ISO 80369-7<br>Male luer lock with filter outlet compliant with ISO 80369-7<br><b>Operating temperature Range:</b> From 5 °C to 40 °C<br><b>Storage temperature Range:</b> From 0 °C to 40 °C<br><b>Maximum applicable pressure:</b> 3,2 bar<br><br><b>Biological:</b><br><b>Biocompatibility:</b> Compliant with ISO 10993-1<br><br><b>Features:</b><br><b>Type of administration:</b> gravity / pressure<br><b>Duration of the application:</b> up to 120 hours<br><b>Filter:</b> Speedflow Adult 0.2+ µm vented<br><b>Filter pore size:</b> 0.2 µm<br><b>Filter internal volume:</b> < 2.4 ml<br><b>Filter media:</b> hydrophilic PES membrane charged with Polyethylenimine and hydrophobic PTFE membrane<br><br><b>Flow Regulator:</b> No<br><b>Drip Chamber:</b> No<br><b>Roller:</b> No<br><b>Y-injection site:</b> No<br><b>Clamp:</b> No<br><b>Tubing:</b> PU tube – inner Ø 1.5 mm / outer Ø 3.0 mm  |
|   | <b>PRODUCT SHELF LIFE</b>   |
| <b>STERILIZATION</b>                        | <b>Sterile:</b> Yes – EtO<br><br><b>Suitable for Sterilization/Re-sterilization:</b> No   |
| <b>APPLICABLE STANDARDS AND REGULATIONS</b> | <b>Product Certification:</b><br>CE mark<br><br><b>Applicable Standards and Technical Regulations:</b><br>EN 556-1 Sterilization of medical devices — Requirements for medical devices to be designated "STERILE" — Part 1: Requirements for terminally sterilized medical devices<br>EN ISO 8536-4 Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed<br>EN ISO 8536-9 Infusion equipment for medical use — Part 9: Fluid lines for single use with pressure infusion equipment<br>EN ISO 8536-11 Infusion equipment for medical use — Part 11: Infusion filters for single use with pressure infusion equipment<br>EN ISO 10993-1 Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process<br>EN ISO 10993-4 Biological evaluation of medical devices — Part 4: Selection of tests for interactions with blood<br>EN ISO 10993-5 Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity<br>EN ISO 10993-7 Biological evaluation of medical devices — Part 7: Ethylene oxide sterilization residuals<br>EN ISO 10993-10 Biological evaluation of medical devices — Part 10: Tests for irritation and skin sensitization<br>EN ISO 10993-11 Biological evaluation of medical devices — Part 11: Tests for systemic toxicity<br>EN ISO 10993-18 Biological evaluation of medical devices — Part 18: Chemical characterization of materials<br>EN ISO 10993-23 Biological evaluation of medical devices — Part 23: Tests for irritation<br>EN ISO 11135 Sterilization of health-care products — Ethylene oxide — Requirements for the development, validation and routine control of a sterilization process for medical devices |

|  |  |
|--|--|
| <b>Product PN</b> GSS021A00S                                     | <b>Mod. 984e-ext</b><br><b>Rev. 07</b> |
| <b>Description</b> HI-FLO Extension Set Endotoxins Adult 0.2+ µm |  |

|                             | <p>EN ISO 11607-1 Packaging for terminally sterilized medical devices — Part 1: Requirements for materials, sterile barrier systems and packaging systems</p> <p>EN ISO 11607-2 Packaging for terminally sterilized medical devices — Part 2: Validation requirements for forming, sealing and assembly processes</p> <p>EN ISO 13485 Medical devices — Quality management systems — Requirements for regulatory purposes</p> <p>EN ISO 14971 Medical devices — Application of risk management to medical devices</p> <p>EN ISO 15223-1 Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied - Part 1: General requirements</p> <p>EN ISO 20417 Medical devices — Information to be supplied by the manufacturer</p> <p>IEC 62366-1 Medical devices — Part 1: Application of usability engineering to medical devices</p> <p>EN ISO 80369-1 Small-bore connectors for liquids and gases in healthcare applications — Part 1: General requirements</p> <p>EN ISO 80369-7 Small-bore connectors for liquids and gases in healthcare applications — Part 7: Connectors for intravascular or hypodermic applications</p> <p>EN ISO 80369-20 Small-bore connectors for liquids and gases in healthcare applications — Part 20: Common test methods</p> |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
|-----------------------------|--|----|-------------|---|--------------------------|---|--|---|---|---|--|---|----------------|---|--------------------|
| <b>INSTRUCTIONS FOR USE</b> | Available languages:<br>English / Italian / German / French / Spanish  |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| <b>PACKAGING</b>            | <p><b>Primary Packaging:</b><br/>Devices are individually packed and label in medical paper bags.<br/>Bag Size: 130 X 200 mm</p> <p><b>Secondary Packaging:</b><br/>Bags are placed inside a microperforated sack.</p> <p><b>Tertiary Packaging:</b><br/>Carton Box.<br/>Box Size: 60 x 40 x 20 cm<br/>Box Weight: 5.5 kg<br/>Devices per box: 300</p>   |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| <b>CERTIFICATIONS</b>       | <p>ISO 9001:2015</p> <p>ISO 13485:2016</p> <p>CE Certificate (2017/745/UE)</p>   |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| <b>DRAWING</b>              | <div style="display: flex; align-items: center;">  <table border="1" style="margin-left: 20px;"> <thead> <tr> <th>ID</th> <th>Description</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>Cap for Female Luer Lock</td> </tr> <tr> <td>2</td> <td>Speedflow Adult 0.2+ IV µm Filter with femeale luer lock</td> </tr> <tr> <td>3</td> <td>Tube 2 cm – inner Ø 2.9 mm / outer Ø 4.1 mm</td> </tr> <tr> <td>4</td> <td>Tube 11 cm – inner Ø 1.5 mm / outer Ø 3.0 mm</td> </tr> <tr> <td>5</td> <td>Male luer lock</td> </tr> <tr> <td>6</td> <td>Female luer filter</td> </tr> </tbody> </table> </div>   | ID | Description | 1 | Cap for Female Luer Lock | 2 | Speedflow Adult 0.2+ IV µm Filter with femeale luer lock | 3 | Tube 2 cm – inner Ø 2.9 mm / outer Ø 4.1 mm | 4 | Tube 11 cm – inner Ø 1.5 mm / outer Ø 3.0 mm | 5 | Male luer lock | 6 | Female luer filter |
| ID                          | Description  |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| 1                           | Cap for Female Luer Lock   |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| 2                           | Speedflow Adult 0.2+ IV µm Filter with femeale luer lock   |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| 3                           | Tube 2 cm – inner Ø 2.9 mm / outer Ø 4.1 mm  |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| 4                           | Tube 11 cm – inner Ø 1.5 mm / outer Ø 3.0 mm   |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| 5                           | Male luer lock   |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |
| 6                           | Female luer filter   |    |             |   |                          |   |  |   |   |   |  |   |                |   |                    |






# PRODUCT SPECIFICATION

CE<sub>0051</sub>

|             |   |                          |
|-------------|---|--------------------------|
| Product PN  | GSS021A00S                                    | Mod. 984e-ext<br>Rev. 07 |
| Description | HI-FLO Extension Set Endotoxins Adult 0.2+ µm |                          |

## REVISIONS AND APPROVALS:

| DATE       | REV. | REASON FOR CHANGE | ISSUED BY:<br>(name/function/signature)  | VERIFIED BY:<br>(name/function/signature)  | APPROVED BY:<br>(name/function/signature)   |
|------------|------|-------------------|--|--|---|
| 26/02/2023 | 00   | First issue       | Barbara Palmieri<br>RA Specialist<br> | Barbara Finessi<br>QA Manage<br> | Luca Zanini<br>VP Healthcare and<br>Lifesience<br> |