

Product PN	GSS021A00S	Mod. 984e-ext
Description	HI-FLO Extension Set Endotoxins Adult 0.2+ µm	Rev. 07

## HI-FLO Extension Set Adult with 0.2 µm Filter positively charged



<b>PRODUCT DESCRIPTION</b>	<p>Extension set for infusion for intravascular applications.</p> <p>The device is sterile and can be used in combination with an infusion set or an infusion device (pump or syringe). The connections are a female luer lock with cap inlet and a male luer lock with 1.2 µm filter outlet, compliant with ISO 80369-7</p> <p>The set is provided with a vented Speedflow® Adult filter, with a hydrophilic PES membrane with 0.2 µm pore size positively charged for particles and bacteria endotoxins retention and a hydrophobic PTFE membrane with 0,03 µm pore size.</p> <p>The approximate total length of the set is 245 mm.</p> <p>The set includes the following components:</p> <ul style="list-style-type: none"> <li>Female luer lock with cap inlet;</li> <li>Speedflow Adult 0.2+ µm IV Filter;</li> <li>Male luer lock with filter outlet.</li> </ul>	
<b>MANUFACTURER NAME</b>	<p><b>GVS SpA</b> Via Roma, 50 40069 Zola Predosa (BO) – ITALY Phone: +39.051.6176311 – Fax: +39.051.6176200 e-mail: <a href="mailto:gvs@gvs.com">gvs@gvs.com</a> – website: <a href="http://www.gvs.com">www.gvs.com</a></p>	
<b>INTENDED USE / APPLICATION</b>	<p>Infusion of Drugs (including chemotherapy), Anesthetics, Nutritional Solutions and Saline Solutions for intravascular applications.</p> <p>The set can be connected via Luer Locks to all commercially available infusion administration sets compliant with ISO 80369-7.</p> <p>The set can be used either for gravity or in combination with an infusion set or an infusion device (pump or syringe).</p> <p>The set is intended specifically to eliminate air bubbles and to retain particles, bacteria and endotoxins.</p> <p>The set is a single-use device that can be used applications that last up to 120 hours.</p> <p>The set has to be disposed after each therapy.</p> <p>The set cannot be used for infusion of hyper alimentation liquids, lipids, blood and/or blood derivatives.</p> <p>The device should only be supervised and used by qualified healthcare personnel.</p>	
<b>CLASS OF THE PRODUCT</b>	<p>Class IIa – sterile – single use Rule 2 and 3 Annex VIII 2017/472/UE</p>	
<b>REGISTRATION NUMBERS</b>	<p><b>Italian national database:</b> <b>GSS021A00S</b> 2439371</p>	
<b>EMDN</b>	<b>A03020101</b>	LOW PRESSURE EXTENSION LINES
<b>MATERIALS</b>	<p><b>Filter media:</b> PES Hydrophilic membrane / PTFE Hydrophobic membrane / Polyethylenimine</p> <p><b>Filter housing:</b> MBS</p> <p><b>Tubes:</b> PU</p> <p><b>Luer Lock:</b> MABS</p> <p><b>Caps:</b> HDPE</p> <p><b>Regulatory Compliance:</b></p> <ul style="list-style-type: none"> <li>Biocompatibility according to ISO 10993-1</li> <li>Rohs directive 2011/65/UE</li> <li>DEHP plasticizer Free</li> <li>Latex free</li> </ul>	



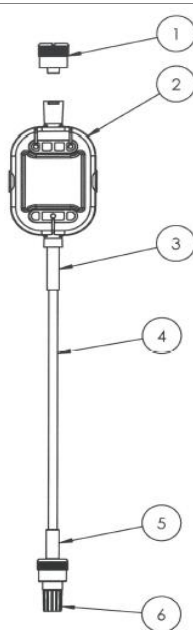
# PRODUCT SPECIFICATION



Product PN	GSS021A00S	Mod. 984e-ext
Description	HI-FLO Extension Set Endotoxins Adult 0.2+ µm	Rev. 07

	<ul style="list-style-type: none"><li>▪ Reach 1907/2006/CE (hazardous substances regulation)</li><li>▪ Reg. 1272/2008/CE (classification, labelling and packaging of substances and mixtures)</li></ul>																										
<b>PRODUCT CHARACTERISTICS</b>	<p><b>Physical/Mechanical:</b></p> <p>Approximate total length: 245 mm</p> <p>Total internal volume of the set: 5 ml</p> <p>Weight: 16 g</p> <p>Input/output connectors: Female luer lock with cap inlet compliant with ISO 80369-7 Male luer lock with filter outlet compliant with ISO 80369-7</p> <p>Operating temperature Range: From 5 °C to 40 °C</p> <p>Storage temperature Range: From 0 °C to 40 °C</p> <p>Maximum applicable pressure: 3,2 bar</p> <p><b>Biological:</b></p> <p>Biocompatibility: Compliant with ISO 10993-1</p> <p><b>Features:</b></p> <p>Type of administration: gravity / pressure</p> <p>Duration of the application: up to 120 hours</p> <p>Filter: Speedflow Adult 0.2+ µm vented</p> <p>Filter pore size: 0.2 µm</p> <p>Filter internal volume: &lt; 2.4 ml</p> <p>Filter media: hydrophilic PES membrane charged with Polyethylenimine and hydrophobic PTFE membrane</p> <p>Flow Regulator: No</p> <p>Drip Chamber: No</p> <p>Roller: No</p> <p>Y-injection site: No</p> <p>Clamp: No</p> <p>Tubing: PU tube – inner Ø 1.5 mm / outer Ø 3.0 mm</p>																										
<b>PRODUCT SHELF LIFE</b>	5 years																										
<b>STERILIZATION</b>	<p><b>Sterile:</b> Yes – EtO</p> <p><b>Suitable for Sterilization/Re-sterilization:</b> No</p>																										
<b>APPLICABLE STANDARDS AND REGULATIONS</b>	<p><b>Product Certification:</b> CE mark</p> <p><b>Applicable Standards and Technical Regulations:</b></p> <table><tr><td>EN 556-1</td><td>Sterilization of medical devices — Requirements for medical devices to be designated "STERILE" — Part 1: Requirements for terminally sterilized medical devices</td></tr><tr><td>EN ISO 8536-4</td><td>Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed</td></tr><tr><td>EN ISO 8536-9</td><td>Infusion equipment for medical use — Part 9: Fluid lines for single use with pressure infusion equipment</td></tr><tr><td>EN ISO 8536-11</td><td>Infusion equipment for medical use — Part 11: Infusion filters for single use with pressure infusion equipment</td></tr><tr><td>EN ISO 10993-1</td><td>Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process</td></tr><tr><td>EN ISO 10993-4</td><td>Biological evaluation of medical devices — Part 4: Selection of tests for interactions with blood</td></tr><tr><td>EN ISO 10993-5</td><td>Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity</td></tr><tr><td>EN ISO 10993-7</td><td>Biological evaluation of medical devices — Part 7: Ethylene oxide sterilization residuals</td></tr><tr><td>EN ISO 10993-10</td><td>Biological evaluation of medical devices — Part 10: Tests for irritation and skin sensitization</td></tr><tr><td>EN ISO 10993-11</td><td>Biological evaluation of medical devices — Part 11: Tests for systemic toxicity</td></tr><tr><td>EN ISO 10993-18</td><td>Biological evaluation of medical devices — Part 18: Chemical characterization of materials</td></tr><tr><td>EN ISO 10993-23</td><td>Biological evaluation of medical devices — Part 23: Tests for irritation</td></tr><tr><td>EN ISO 11135</td><td>Sterilization of health-care products — Ethylene oxide — Requirements for the development, validation and routine control of a sterilization process for medical devices</td></tr></table>	EN 556-1	Sterilization of medical devices — Requirements for medical devices to be designated "STERILE" — Part 1: Requirements for terminally sterilized medical devices	EN ISO 8536-4	Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed	EN ISO 8536-9	Infusion equipment for medical use — Part 9: Fluid lines for single use with pressure infusion equipment	EN ISO 8536-11	Infusion equipment for medical use — Part 11: Infusion filters for single use with pressure infusion equipment	EN ISO 10993-1	Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process	EN ISO 10993-4	Biological evaluation of medical devices — Part 4: Selection of tests for interactions with blood	EN ISO 10993-5	Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity	EN ISO 10993-7	Biological evaluation of medical devices — Part 7: Ethylene oxide sterilization residuals	EN ISO 10993-10	Biological evaluation of medical devices — Part 10: Tests for irritation and skin sensitization	EN ISO 10993-11	Biological evaluation of medical devices — Part 11: Tests for systemic toxicity	EN ISO 10993-18	Biological evaluation of medical devices — Part 18: Chemical characterization of materials	EN ISO 10993-23	Biological evaluation of medical devices — Part 23: Tests for irritation	EN ISO 11135	Sterilization of health-care products — Ethylene oxide — Requirements for the development, validation and routine control of a sterilization process for medical devices
EN 556-1	Sterilization of medical devices — Requirements for medical devices to be designated "STERILE" — Part 1: Requirements for terminally sterilized medical devices																										
EN ISO 8536-4	Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed																										
EN ISO 8536-9	Infusion equipment for medical use — Part 9: Fluid lines for single use with pressure infusion equipment																										
EN ISO 8536-11	Infusion equipment for medical use — Part 11: Infusion filters for single use with pressure infusion equipment																										
EN ISO 10993-1	Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process																										
EN ISO 10993-4	Biological evaluation of medical devices — Part 4: Selection of tests for interactions with blood																										
EN ISO 10993-5	Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity																										
EN ISO 10993-7	Biological evaluation of medical devices — Part 7: Ethylene oxide sterilization residuals																										
EN ISO 10993-10	Biological evaluation of medical devices — Part 10: Tests for irritation and skin sensitization																										
EN ISO 10993-11	Biological evaluation of medical devices — Part 11: Tests for systemic toxicity																										
EN ISO 10993-18	Biological evaluation of medical devices — Part 18: Chemical characterization of materials																										
EN ISO 10993-23	Biological evaluation of medical devices — Part 23: Tests for irritation																										
EN ISO 11135	Sterilization of health-care products — Ethylene oxide — Requirements for the development, validation and routine control of a sterilization process for medical devices																										

<b>Product PN</b>	<b>GSS021A00S</b>	<b>Mod. 984e-ext</b>  <b>Rev. 07</b>
<b>Description</b>	<b>HI-FLO Extension Set Endotoxins Adult 0.2+ µm</b>	

	<p>EN ISO 11607-1 Packaging for terminally sterilized medical devices — Part 1: Requirements for materials, sterile barrier systems and packaging systems</p> <p>EN ISO 11607-2 Packaging for terminally sterilized medical devices — Part 2: Validation requirements for forming, sealing and assembly processes</p> <p>EN ISO 13485 Medical devices — Quality management systems — Requirements for regulatory purposes</p> <p>EN ISO 14971 Medical devices — Application of risk management to medical devices</p> <p>EN ISO 15223-1 Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied - Part 1: General requirements</p> <p>EN ISO 20417 Medical devices — Information to be supplied by the manufacturer</p> <p>IEC 62366-1 Medical devices — Part 1: Application of usability engineering to medical devices</p> <p>EN ISO 80369-1 Small-bore connectors for liquids and gases in healthcare applications — Part 1: General requirements</p> <p>EN ISO 80369-7 Small-bore connectors for liquids and gases in healthcare applications — Part 7: Connectors for intravascular or hypodermic applications</p> <p>EN ISO 80369-20 Small-bore connectors for liquids and gases in healthcare applications — Part 20: Common test methods</p>														
<b>INSTRUCTIONS FOR USE</b>	<p><b>Available languages:</b> English / Italian / German / French / Spanish / Hungarian / Romanian</p>														
<b>PACKAGING</b>	<p><b>Primary Packaging:</b> Devices are individually packed and label in medical paper bags. Bag Size: 130 X 200 mm</p> <p><b>Secondary Packaging:</b> Bags are placed inside a microperforated sack.</p> <p><b>Tertiary Packaging:</b> Carton Box. Box Size: 60 x 40 x 20 cm Box Weight: 5.5 kg Devices per box: 300</p>														
<b>CERTIFICATIONS</b>	<p><b>ISO 9001:2015</b> <b>ISO 13485:2016</b> <b>CE Certificate (2017/745/UE)</b></p>														
<b>DRAWING</b>	<div>  <table border="1"> <thead> <tr> <th>ID</th><th>Description</th></tr> </thead> <tbody> <tr> <td>1</td><td>Cap for Female Luer Lock</td></tr> <tr> <td>2</td><td>Speedflow Adult 0.2+ IV µm Filter with female luer lock</td></tr> <tr> <td>3</td><td>Tube 2 cm – inner Ø 2.9 mm / outer Ø 4.1 mm</td></tr> <tr> <td>4</td><td>Tube 11 cm – inner Ø 1.5 mm / outer Ø 3.0 mm</td></tr> <tr> <td>5</td><td>Male luer lock</td></tr> <tr> <td>6</td><td>Female luer filter</td></tr> </tbody> </table> </div>	ID	Description	1	Cap for Female Luer Lock	2	Speedflow Adult 0.2+ IV µm Filter with female luer lock	3	Tube 2 cm – inner Ø 2.9 mm / outer Ø 4.1 mm	4	Tube 11 cm – inner Ø 1.5 mm / outer Ø 3.0 mm	5	Male luer lock	6	Female luer filter
ID	Description														
1	Cap for Female Luer Lock														
2	Speedflow Adult 0.2+ IV µm Filter with female luer lock														
3	Tube 2 cm – inner Ø 2.9 mm / outer Ø 4.1 mm														
4	Tube 11 cm – inner Ø 1.5 mm / outer Ø 3.0 mm														
5	Male luer lock														
6	Female luer filter														





# PRODUCT SPECIFICATION

CE 0051

Product PN	GSS021A00S	Mod. 984e-ext Rev. 07
Description	HI-FLO Extension Set Endotoxins Adult 0.2+ µm	

## REVISIONS AND APPROVALS:

DATE	REV.	REASON FOR CHANGE	ISSUED BY: (name/function/signature)	VERIFIED BY: (name/function/signature)	APPROVED BY: (name/function/signature)
14/02/2025	02	Added Hungarian and Romanian translations on labels and IFU	Barbara Palmieri RA Specialist 	Barbara Finessi QA Manage 	Luca Zanini VP Healthcare and Lifesience 