

Product PN GMD015A00S GMD016A00S GMD017A00S GMD018A00S

Mod. 984e-ext

Description Speedflow® IV Filter Neonatal 0.2/0.2+/1.2/5.0 µm

Rev. 07

Speedflow® Filter Neonatal 0.2/0.2+/1.2/5.0 µm



PRODUCT DESCRIPTION	Vented filter for infusion and anaesthesia. The device is sterile and can be used in combination with an infusion set or an infusion device (pump or syringe). The connections are a female luer lock with vented cap inlet and a rotating male luer lock with vented cap outlet, compliant with ISO 80369-7. The device is provided with a vented Speedflow® Neonatal filter, with an hydrophilic PES membrane with 0.2/0.2+/1.2/5.0 µm pore size for particles retention and a hydrophobic PTFE membrane with 0,03 µm pore size. The filter size (LxWxH) is 15.3x62x9.6 mm.
CONFIGURATIONS	GMD015A00S 0.2 µm GMD016A00S 0.2+ (positively charged) µm GMD017A00S 1.2 µm GMD018A00S 5.0 µm
MANUFACTURER NAME	GVS S.p.A. Via Roma, 50 – 40069 Zola Predosa (BO) – Italy Phone: +39.051.6176311 – Fax: +39.051.6176200 email: gvs@gvs.it – website: www.gvs.com
INTENDED USE / APPLICATION	Infusion of Drugs (including chemotherapy), Anesthetics, Nutritional Solutions and Saline Solutions. The set can be connected via Luer Locks to all commercially available infusion administration sets compliant with ISO 80369-7. The filter can be used in combination with an infusion set or an infusion device (pump or syringe). The device is intended to retain different particles depending on its filter pore size: <ul style="list-style-type: none">▪ 0.2 µm filter is intended specifically to eliminate air bubbles and to retain particles and bacteria,▪ 1.2 µm filter is intended specifically to eliminate air bubbles and to retain fungi and microorganisms,▪ 0.2+ µm filter is intended specifically to eliminate air bubbles and to retain particles, bacteria and endotoxins,▪ 5.0 µm filter is intended specifically to eliminate air bubbles and to retain particles. The device is a single-use device that can be used applications that last: <ul style="list-style-type: none">▪ Devices with 0.2 µm filter: up to 96 hours;▪ Devices with 1.2 µm filter: up to 24 hours;▪ Devices with 0.2+ µm filter: up to 120 hours. The device has to be disposed after each therapy. Devices with 0.2/0.2+ µm filter cannot be used for infusion of hyper alimentation liquids, lipids, blood and/or blood derivatives. Devices with 1.2 µm filter cannot be used for infusion of blood and/or blood derivatives. Devices with 5.0 µm filter cannot be used for infusion therapy without further bacterial retention filter. The device should only be supervised and used by qualified healthcare personnel.
CLASS OF THE PRODUCT	Class IIa – sterile – single use Rule 3 Annex VIII 2017/472/UE
REGISTRATION NUMBERS	Italian national database: GMD015A00S 2436399 GMD016A00S 2436705 GMD017A00S 2436707 GMD018A00S 2436708
EMDN	A04010101 WITHDRAWL AND ADMINISTRATION FILTERS (0.2-1.2 MICRONS) A04010102 ASPIRATION AND TRANSFER FILTERS (>= 5 MICRONS)
MATERIALS	Filter media: PES Hydrophilic membrane / PTFE Hydrophobic membrane / 0.2+ filters include also Polyethylenimine Filter housing: MBS / PP



PRODUCT SPECIFICATION

CE 0051

Product PN GMD015A00S GMD016A00S GMD017A00S GMD018A00S

Mod. 984e-ext

Description Speedflow® IV Filter Neonatal 0.2/0.2+/1.2/5.0 µm

Rev. 07

	<p>Caps: HDPE</p> <p>Regulatory Compliance:</p> <ul style="list-style-type: none">▪ Biocompatibility according to ISO 10993-1▪ RoHS directive 2011/65/UE▪ DEHP plasticizer Free▪ Latex free▪ Reach 1907/2006/CE (hazardous substances regulation)▪ Reg. 1272/2008/CE (classification, labelling and packaging of substances and mixtures)																						
PRODUCT CHARACTERISTICS	<p>Physical/Mechanical:</p> <p>Dimensions (LxWxH): 15.3x62x9.6 mm</p> <p>Total internal volume of the set: < 0.35 ml</p> <p>Weight: 2.56 g</p> <p>Input/output connectors: Female luer lock with vented cap inlet and rotating male luer lock with vented cap outlet, compliant with ISO 80369-7</p> <p>Operating temperature Range: From 5 °C to 40 °C</p> <p>Storage temperature Range: From 0 °C to 40 °C</p> <p>Maximum applicable pressure: 3.2 bar</p> <p>Flow Rate:</p> <table><tr><td>0.2 µm:</td><td>≥ 4 ml/min @ 80 cm (31.5 in) water head pressure</td></tr><tr><td>0.2 µm+:</td><td>≥ 3.5 ml/min @ 80 cm (31.5 in) water head pressure</td></tr><tr><td>1.2 µm:</td><td>≥ 30 ml/min @ 80 cm (31.5 in) water head pressure</td></tr><tr><td>5.0 µm:</td><td>≥ 55 ml/min @ 80 cm (31.5 in) water head pressure</td></tr></table> <p>Bubble point:</p> <table><tr><td>0.2 µm:</td><td>3.7 ÷ 4.8 bar</td></tr><tr><td>0.2 µm+:</td><td>3.7 ÷ 4.8 bar</td></tr><tr><td>1.2 µm:</td><td>0.7 ÷ 1.0 bar</td></tr><tr><td>5.0 µm:</td><td>0.15 ÷ 0.3 bar</td></tr></table> <p>Biological:</p> <p>Biocompatibility: Compliant with ISO 10993-1</p> <p>Features:</p> <p>Type of administration: gravity / pressure</p> <p>Duration of the application:</p> <table><tr><td>0.2 µm</td><td>up to 96 hours</td></tr><tr><td>1.2 µm</td><td>up to 24 hours</td></tr><tr><td>0.2+ µm</td><td>up to 120 hours</td></tr></table> <p>Filter: Speedflow Neonatal 0.2/1.2/0.2+/5.0 µm vented</p> <p>Filter pore size: 0.2/1.2/0.2+/5.0 µm</p> <p>Filter internal volume: < 0.35 ml</p> <p>Filter media: hydrophilic PES membrane and hydrophobic PTFE membrane, 0.2+ filters include also Polyethylenimine</p>	0.2 µm:	≥ 4 ml/min @ 80 cm (31.5 in) water head pressure	0.2 µm+:	≥ 3.5 ml/min @ 80 cm (31.5 in) water head pressure	1.2 µm:	≥ 30 ml/min @ 80 cm (31.5 in) water head pressure	5.0 µm:	≥ 55 ml/min @ 80 cm (31.5 in) water head pressure	0.2 µm:	3.7 ÷ 4.8 bar	0.2 µm+:	3.7 ÷ 4.8 bar	1.2 µm:	0.7 ÷ 1.0 bar	5.0 µm:	0.15 ÷ 0.3 bar	0.2 µm	up to 96 hours	1.2 µm	up to 24 hours	0.2+ µm	up to 120 hours
0.2 µm:	≥ 4 ml/min @ 80 cm (31.5 in) water head pressure																						
0.2 µm+:	≥ 3.5 ml/min @ 80 cm (31.5 in) water head pressure																						
1.2 µm:	≥ 30 ml/min @ 80 cm (31.5 in) water head pressure																						
5.0 µm:	≥ 55 ml/min @ 80 cm (31.5 in) water head pressure																						
0.2 µm:	3.7 ÷ 4.8 bar																						
0.2 µm+:	3.7 ÷ 4.8 bar																						
1.2 µm:	0.7 ÷ 1.0 bar																						
5.0 µm:	0.15 ÷ 0.3 bar																						
0.2 µm	up to 96 hours																						
1.2 µm	up to 24 hours																						
0.2+ µm	up to 120 hours																						
PRODUCT SHELF LIFE	5 years																						
STERILIZATION	<p>Sterile: Yes – EtO</p> <p>Suitable for Sterilization/Re-sterilization: No</p>																						
APPLICABLE STANDARDS AND REGULATIONS	<p>Product Certification: CE mark</p> <p>Applicable Standards and Technical Regulations:</p> <table><tr><td>EN 556-1</td><td>Sterilization of medical devices — Requirements for medical devices to be designated "STERILE" — Part 1: Requirements for terminally sterilized medical devices</td></tr><tr><td>EN ISO 8536-4</td><td>Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed</td></tr><tr><td>EN ISO 8536-11</td><td>Infusion equipment for medical use — Part 11: Infusion filters for single use with pressure infusion equipment</td></tr><tr><td>EN ISO 8536-13</td><td>Infusion equipment for medical use — Part 13: Graduated flow regulators for single use with fluid contact</td></tr><tr><td>EN ISO 8536-14</td><td>Infusion equipment for medical use — Part 14: Clamps and flow regulators for transfusion and infusion equipment without fluid contact</td></tr></table>	EN 556-1	Sterilization of medical devices — Requirements for medical devices to be designated "STERILE" — Part 1: Requirements for terminally sterilized medical devices	EN ISO 8536-4	Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed	EN ISO 8536-11	Infusion equipment for medical use — Part 11: Infusion filters for single use with pressure infusion equipment	EN ISO 8536-13	Infusion equipment for medical use — Part 13: Graduated flow regulators for single use with fluid contact	EN ISO 8536-14	Infusion equipment for medical use — Part 14: Clamps and flow regulators for transfusion and infusion equipment without fluid contact												
EN 556-1	Sterilization of medical devices — Requirements for medical devices to be designated "STERILE" — Part 1: Requirements for terminally sterilized medical devices																						
EN ISO 8536-4	Infusion equipment for medical use — Part 4: Infusion sets for single use, gravity feed																						
EN ISO 8536-11	Infusion equipment for medical use — Part 11: Infusion filters for single use with pressure infusion equipment																						
EN ISO 8536-13	Infusion equipment for medical use — Part 13: Graduated flow regulators for single use with fluid contact																						
EN ISO 8536-14	Infusion equipment for medical use — Part 14: Clamps and flow regulators for transfusion and infusion equipment without fluid contact																						



PRODUCT SPECIFICATION

CE 0051

Product PN GMD015A00S GMD016A00S GMD017A00S GMD018A00S

Mod. 984e-ext

Description Speedflow® IV Filter Neonatal 0.2/0.2+/1.2/5.0 µm

Rev. 07

	EN ISO 10993-1	Biological evaluation of medical devices — Part 1: Evaluation and testing within a risk management process
	EN ISO 10993-4	Biological evaluation of medical devices — Part 4: Selection of tests for interactions with blood
	EN ISO 10993-5	Biological evaluation of medical devices — Part 5: Tests for in vitro cytotoxicity
	EN ISO 10993-7	Biological evaluation of medical devices — Part 7: Ethylene oxide sterilization residuals
	EN ISO 10993-10	Biological evaluation of medical devices — Part 10: Tests for irritation and skin sensitization
	EN ISO 10993-11	Biological evaluation of medical devices — Part 11: Tests for systemic toxicity
	EN ISO 10993-18	Biological evaluation of medical devices — Part 18: Chemical characterization of materials
	EN ISO 10993-23	Biological evaluation of medical devices — Part 23: Tests for irritation
	EN ISO 11135	Sterilization of health-care products — Ethylene oxide — Requirements for the development, validation and routine control of a sterilization process for medical devices
	EN ISO 11607-1	Packaging for terminally sterilized medical devices — Part 1: Requirements for materials, sterile barrier systems and packaging systems
	EN ISO 11607-2	Packaging for terminally sterilized medical devices — Part 2: Validation requirements for forming, sealing and assembly processes
	EN ISO 13485	Medical devices — Quality management systems — Requirements for regulatory purposes
	EN ISO 14971	Medical devices — Application of risk management to medical devices
	EN ISO 15223-1	Medical devices — Symbols to be used with medical device labels, labelling and information to be supplied — Part 1: General requirements
	EN ISO 20417	Medical devices — Information to be supplied by the manufacturer
	IEC 62366-1	Medical devices — Part 1: Application of usability engineering to medical devices
	EN ISO 80369-1	Small-bore connectors for liquids and gases in healthcare applications — Part 1: General requirements
	EN ISO 80369-7	Small-bore connectors for liquids and gases in healthcare applications — Part 7: Connectors for intravascular or hypodermic applications
	EN ISO 80369-20	Small-bore connectors for liquids and gases in healthcare applications — Part 20: Common test methods
INSTRUCTIONS FOR USE	Available languages:	English / Italian / German / French / Spanish / Hungarian / Romanian
PACKAGING	Primary Packaging:	Devices are individually packed and label in medical paper bags. Bag Size: 100 X 145 mm
	Secondary Packaging:	Bags are placed inside a microperforated sack.
	Tertiary Packaging:	Carton Box. Box Size: 60 x 40 x 20 cm Box Weight: 4 kg Devices per box: 400
CERTIFICATIONS	ISO 9001:2015 ISO 13485:2016 CE Certificate (2017/745/UE)	


Product PN GMD015A00S GMD016A00S GMD017A00S GMD018A00S

Mod. 984e-ext

Description Speedflow® IV Filter Neonatal 0.2/0.2+/1.2/5.0 µm

Rev. 07

DRAWING

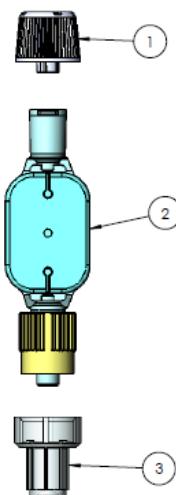

ID	Description
1	Vented male rotating cap for female Luer Lock
2	'15' model: Speedflow Neonatal 0.2 µm IV filter vented '16' model: Speedflow Neonatal 0.2+ µm IV filter vented '17' model: Speedflow Neonatal 1.2 µm IV filter vented '18' model: Speedflow Neonatal 5.0 µm IV filter vented
3	Vented protecting cap for rotating male Luer Lock

REVISIONS AND APPROVALS:

DATE	REV.	REASON FOR CHANGE	ISSUED BY: (name/function/signature)	VERIFIED BY: (name/function/signature)	APPROVED BY: (name/function/signature)
14/02/2025	02	Added Hungarian and Romanian translations on labels and IFU	Barbara Palmieri RA Specialist 	Barbara Finessi QA Manage 	Luca Zanini VP Healthcare and Lifesience